



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

| APPLICATION NO. | FILING DATE | FIRST NAMED INVENTOR | ATTORNEY DOCKET NO. | CONFIRMATION NO. |
|-----------------|-------------|----------------------|---------------------|------------------|
| 10/823,408 | 04/13/2004 | Susumu Moriya | 0388-043850 | 3243 |

7590 11/23/2005

Russell D. Orkin
WEBB ZIESENHEIM LOGSDON ORKIN & HANSON, P.C.
700 Koppers Building
436 Seventh Avenue
Pittsburgh, PA 15219-1818

EXAMINER

HESS, DOUGLAS A

| ART UNIT | PAPER NUMBER |
|----------|--------------|
|----------|--------------|

3651

DATE MAILED: 11/23/2005

Please find below and/or attached an Office communication concerning this application or proceeding.

Office Action Summary

Application No.

10/823,408

Applicant(s)

MORIYA ET AL.

Examiner

Douglas A. Hess

Art Unit

3651

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address --

Period for Reply

A SHORTENED STATUTORY PERIOD FOR REPLY IS SET TO EXPIRE 3 MONTH(S) OR THIRTY (30) DAYS, WHICHEVER IS LONGER, FROM THE MAILING DATE OF THIS COMMUNICATION.

- Extensions of time may be available under the provisions of 37 CFR 1.136(a). In no event, however, may a reply be timely filed after SIX (6) MONTHS from the mailing date of this communication.
- If NO period for reply is specified above, the maximum statutory period will apply and will expire SIX (6) MONTHS from the mailing date of this communication.
- Failure to reply within the set or extended period for reply will, by statute, cause the application to become ABANDONED (35 U.S.C. § 133). Any reply received by the Office later than three months after the mailing date of this communication, even if timely filed, may reduce any earned patent term adjustment. See 37 CFR 1.704(b).

Status

- 1) ☒ Responsive to communication(s) filed on 27 September 2005.
- 2a) ☒ This action is **FINAL**. 2b) ☐ This action is non-final.
- 3) ☐ Since this application is in condition for allowance except for formal matters, prosecution as to the merits is closed in accordance with the practice under *Ex parte Quayle*, 1935 C.D. 11, 453 O.G. 213.

Disposition of Claims

- 4) ☒ Claim(s) 1-3, 5, 10, 14-19 and 21-28 is/are pending in the application.
- 4a) Of the above claim(s) _____ is/are withdrawn from consideration.
- 5) ☒ Claim(s) 1-3, 5, 10, 14-19 and 21-25 is/are allowed.
- 6) ☒ Claim(s) 26-28 is/are rejected.
- 7) ☐ Claim(s) _____ is/are objected to.
- 8) ☐ Claim(s) _____ are subject to restriction and/or election requirement.

Application Papers

- 9) ☐ The specification is objected to by the Examiner.
- 10) ☐ The drawing(s) filed on _____ is/are: a) ☐ accepted or b) ☐ objected to by the Examiner.
Applicant may not request that any objection to the drawing(s) be held in abeyance. See 37 CFR 1.85(a).
Replacement drawing sheet(s) including the correction is required if the drawing(s) is objected to. See 37 CFR 1.121(d).
- 11) ☐ The oath or declaration is objected to by the Examiner. Note the attached Office Action or form PTO-152.

Priority under 35 U.S.C. § 119

- 12) ☒ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
- a) ☒ All b) ☐ Some * c) ☐ None of:
1. ☒ Certified copies of the priority documents have been received.
 2. ☐ Certified copies of the priority documents have been received in Application No. _____.
 3. ☐ Copies of the certified copies of the priority documents have been received in this National Stage application from the International Bureau (PCT Rule 17.2(a)).

* See the attached detailed Office action for a list of the certified copies not received.

Attachment(s)

- 1) ☒ Notice of References Cited (PTO-892)
- 2) ☐ Notice of Draftsperson's Patent Drawing Review (PTO-948)
- 3) ☐ Information Disclosure Statement(s) (PTO-1449 or PTO/SB/08)
Paper No(s)/Mail Date _____

- 4) ☐ Interview Summary (PTO-413)
Paper No(s)/Mail Date. _____

- 5) ☐ Notice of Informal Patent Application (PTO-152)

- 6) ☒ Other: Pages 7, 8 of Nagate et al. & FIG. 4A of Adam et al.

DETAILED ACTION

Claim Rejections - 35 USC § 103

1. The following is a quotation of 35 U.S.C. 103(a) which forms the basis for all obviousness rejections set forth in this Office action:

(a) A patent may not be obtained though the invention is not identically disclosed or described as set forth in section 102 of this title, if the differences between the subject matter sought to be patented and the prior art are such that the subject matter as a whole would have been obvious at the time the invention was made to a person having ordinary skill in the art to which said subject matter pertains. Patentability shall not be negated by the manner in which the invention was made.

2. This application currently names joint inventors. In considering patentability of the claims under 35 U.S.C. 103(a), the examiner presumes that the subject matter of the various claims was commonly owned at the time any inventions covered therein were made absent any evidence to the contrary. Applicant is advised of the obligation under 37 CFR 1.56 to point out the inventor and invention dates of each claim that was not commonly owned at the time a later invention was made in order for the examiner to consider the applicability of 35 U.S.C. 103(c) and potential 35 U.S.C. 102(e), (f) or (g) prior art under 35 U.S.C. 103(a).

3. Claims 26-28 are rejected under 35 U.S.C. 103(a) as being unpatentable over Nagate et al. JP 2002-151571.

Nagate et al. Teach the claimed invention as shown on the attached marked up drawing sheets 7 and 8. Nagate et al. Fail to teach the specifics of the location of his fan/air supply. Nagate et al does show an air supply at 23 in figure 5. It would have been obvious to one of ordinary skill in the art at the time the invention was made to enclose the air supply within the same housing as the filter for the purpose of making the unit more portable and requiring less

Art Unit: 3651

space. Although Nagate et al. does not show any particulars of his air supply, it may even be in the same housing as claimed.

4. Claim 26 is rejected under 35 U.S.C. 103(a) as being unpatentable over Adam et al. USP 6,676,365.

Adam et al. Teach the claimed invention as shown on the attached marked up drawing figure 4A. Adam et al. Fail to teach the specifics of the location of his fan/air supply. Adam et al does show an air supply at 414 in figure 4B. It would have been obvious to one of ordinary skill in the art at the time the invention was made to enclose the air supply within the same housing as the filter for the purpose of making the unit more portable and requiring less space. Although Adam et al. does not show any particulars of his air supply, it may even be in the same housing as claimed.

Allowable Subject Matter

5. Claims 1-3, 5, 10, 14-19, and 21-25 are allowed.

Conclusion

6. Applicant's arguments with respect to claims 26-28 have been considered but are moot in view of the new ground(s) of rejection.

Art Unit: 3651

7. Applicant's amendment necessitated the new ground(s) of rejection presented in this Office action. Accordingly, **THIS ACTION IS MADE FINAL**. See MPEP § 706.07(a). Applicant is reminded of the extension of time policy as set forth in 37 CFR 1.136(a).


A shortened statutory period for reply to this final action is set to expire **THREE MONTHS** from the mailing date of this action. In the event a first reply is filed within **TWO MONTHS** of the mailing date of this final action and the advisory action is not mailed until after the end of the **THREE-MONTH** shortened statutory period, then the shortened statutory period will expire on the date the advisory action is mailed, and any extension fee pursuant to 37 CFR 1.136(a) will be calculated from the mailing date of the advisory action. In no event, however, will the statutory period for reply expire later than **SIX MONTHS** from the date of this final action.

8. Any inquiry concerning this communication or earlier communications from the examiner should be directed to Douglas A. Hess whose telephone number is 571-272-6915. The examiner can normally be reached on M-Thurs 5:30 - 4:00.

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, Gene Crawford can be reached on 571-272-6911. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Art Unit: 3651

9. Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see <http://pair-direct.uspto.gov>. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free).



Douglas A Hess
Primary Examiner
Art Unit 3651

11/17/05

DAH
November 17, 2005

ADAM ET AL.

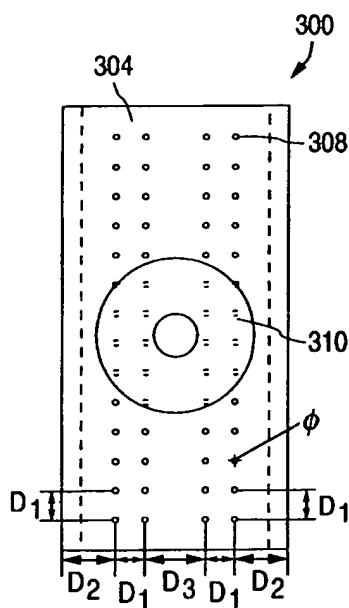


FIG. 3C

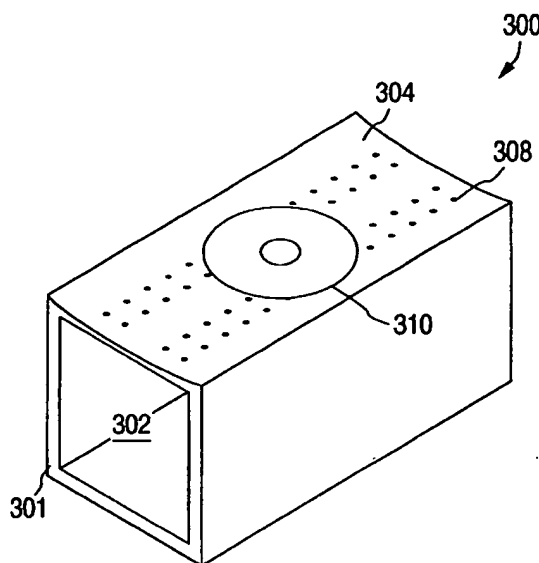


FIG. 3D


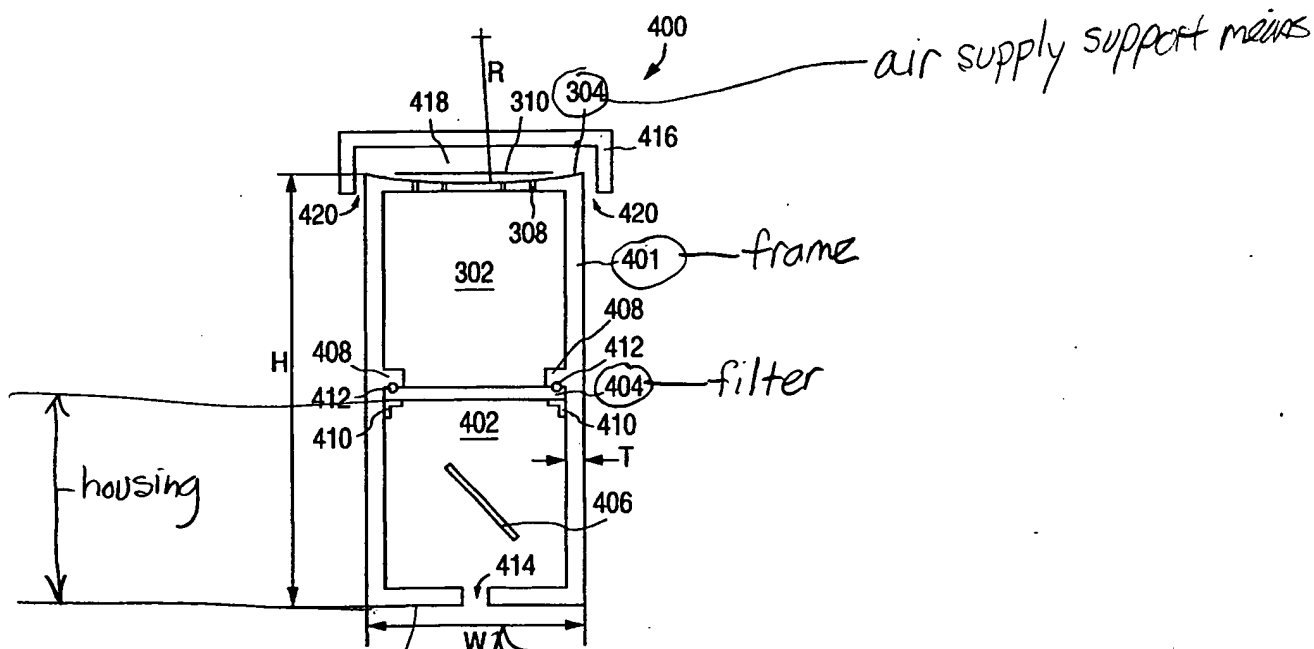


FIG. 4A


fan could be attached here making a single air supply unit

inherent fan provides
air @ inlet 414
could be attached
@ bottom of frame

【図 1】

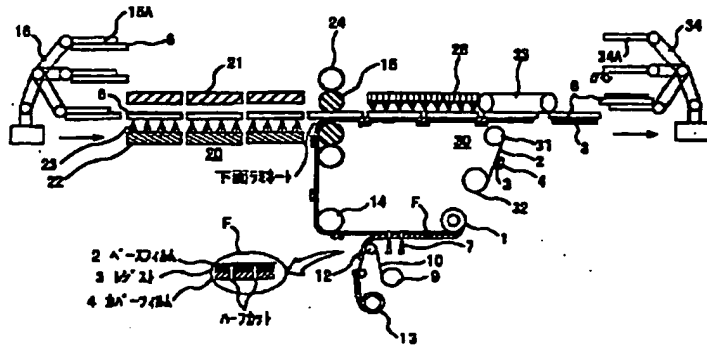


【図 2】

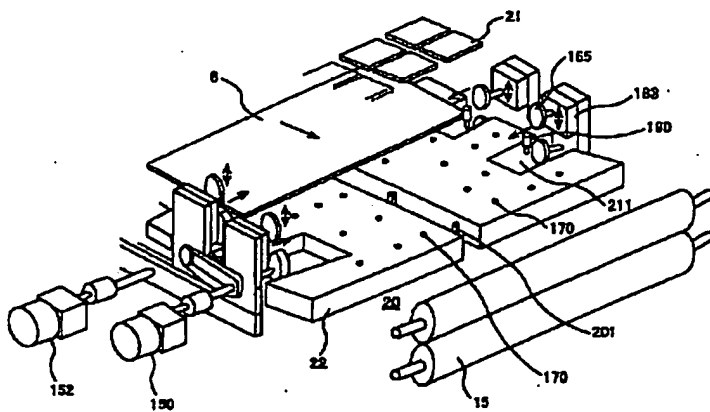

【図 5】

図 5

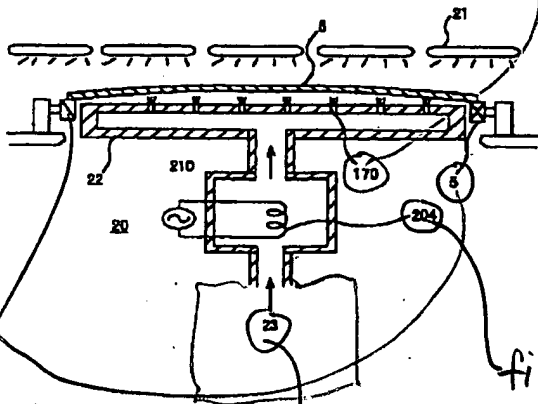


drive rotor

air supply support means

【図 6】


図 6

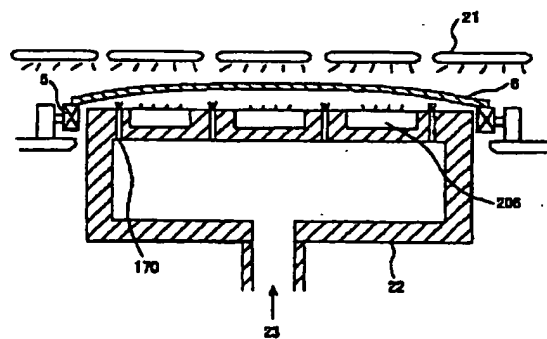

air supply means may be in same unit


【図7】

図 7

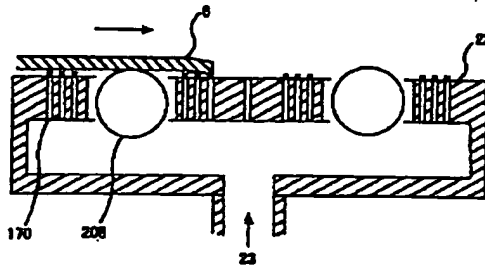


【図8】


図 8

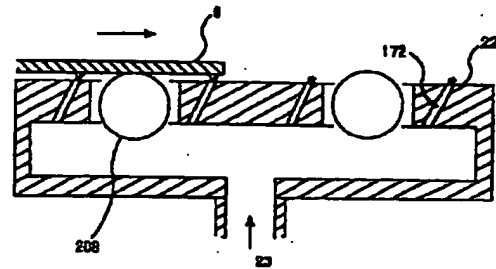

【図9】

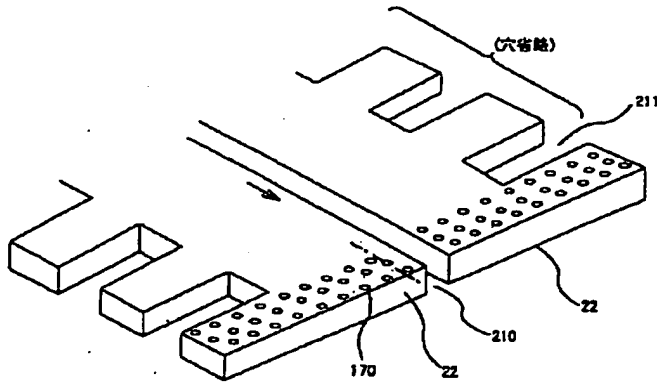

【図10】

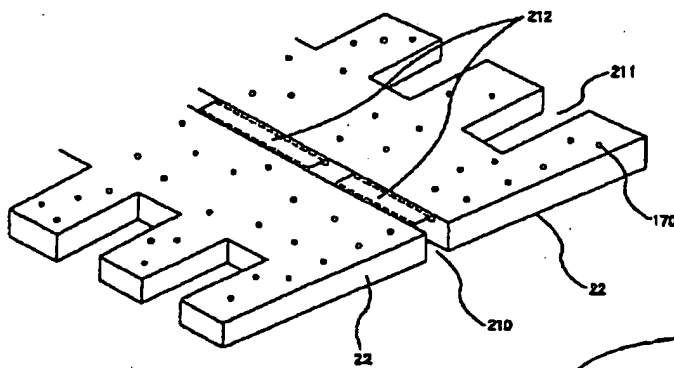

plurality of
units side by side